



TN-0146

Analysis of PFAS in Drinking Water by EPA Method 537.1: A Direct Comparison of the Accuracy and Precision of Manual and Automated SPE Sample Preparation

Dr. David Kennedy¹, Lily Sanchez², Prem Parmar², Sam Lodge¹, and Dr. Bryan Tackett¹

¹Phenomenex, Inc., 411 Madrid Ave., Torrance, CA 90501 USA

²Orange County Water District, 18700 Ward St, Fountain Valley, CA 92708 USA

Introduction

Method 537.1 is a solid phase extraction (SPE) liquid chromatography in tandem with mass spectrometry (LC-MS/MS) method for the determination of selected per- and polyfluorinated alkyl substances (PFAS) in drinking water. Method 537.1 will be part of the upcoming UCMR5, with a focus on PFAS. A critical part of the method is the SPE sample preparation-concentration step which employs a Styrene-DVB copolymer in tube format. Proper performance of this sample preparation step is essential for producing accurate and precise laboratory results. Laboratories can use either a manual or an automated SPE procedure. Therefore, laboratories trying to decide which procedure to deploy may wish to know how well the two techniques perform regarding the expected accuracy and precision of analytical results. In this technical note, we enlisted the assistance of the Orange County Water District (OCWD), a well-regarded drinking water laboratory highly experienced in the application of EPA Method 537.1, to make a direct comparison of the two techniques.

Automated SPE Protocol

Instrumentation:	PromoChrom Technologies SPE-03 Automated SPE System with MOD-004 (sample bottle rinsing) and MOD-005 (minimal Teflon option).
Sample Volume:	250 mL
SPE Cartridge:	Strata® SDB-L; 500 mg/6 mL (Part No. 8B-S014-HCH)
Solvent 1:	Methanol
Solvent 2:	Milli-Q® water
Sample Extraction:	See Table 1.
Extract Concentration:	Concentration Settings: Temperature = 55 °C, Pressure = 10 psi
Concentrate:	Eluate to dryness and allow to cool for 1 minute.
Add:	1 mL of methanol/water (96:4, v/v) to the concentration tube with a micro pipette.
Add:	10 µL of IS-working standard and apply a gentle vortex.
Transfer:	To three polypropylene vials with starburst caps.
Store:	Remaining extracts in centrifuge tubes.

Manual SPE Protocol

Instrumentation:	Vac Elut™ 20 vacuum extraction manifold with vacuum pump.
SPE Cartridge:	Strata SDB-L; 500 mg/6 mL (Part No. 8B-S014-HCH)
Cartridge Clean Up and Conditioning:	Rinse: Cartridge with 3 aliquots of 5 mL methanol. Rinse: Cartridge with 3 aliquots of 6 mL Milli-Q water. Add: 4 mL Milli-Q water to the top of the cartridge.
Sample Extraction:	Fill: Reservoirs with sample before turning on vacuum. Adjust: Pressure to give a 10-15 mL/min flow rate (25-30 min/sample). Stop: Flow with about 10 mL remaining in the reservoirs and rinse the sample bottle with 8 mL Milli-Q water and add to reservoirs. Repeat this step again. Pull: Air through cartridge for 10 min at high vacuum (10-15 in. Hg).
Cartridge Elution:	Turn Off: And release vacuum. Place: Collection tubes into the extraction manifold. Rinse: Sample bottle with 4 mL methanol (swirl down the sides of the reservoir). Reduce: The vacuum power (5 mL/min) so the solvent exits the cartridge in a slow, drop-wise fashion. Do NOT completely dry the cartridge. Repeat: Elution step, but dry cartridge completely. Transfer: Eluents to concentration tubes. Rinse: Collection tubes with 3 mL methanol and add to the concentration tubes. Repeat: Prior rinse again.
Extract Concentration:	Concentration Settings: Temperature = 55 °C, Pressure = 10 psi
Concentrate:	Eluate to dryness and allow to cool for 1 minute.
Add:	1 mL of methanol/water (96:4, v/v) to the concentration tube with a micro pipette.
Add:	10 µL of IS-working standard and apply a gentle vortex.
Transfer:	To three polypropylene vials with starburst caps.
Store:	Remaining extracts in centrifuge tubes.



Table 1. PromoChrom SPE-03 Extraction Procedure

Step	Action	Inlet	Flow Rate (mL/min)	Volume (mL)	Time (min)
1	Elute W2	Solvent 1	5	5	-
2	Wait	-	-	-	1
3	Elute W2	Solvent 1	3	5	-
4	Wait	-	-	-	1
5	Elute W2	Solvent 1	3	5	-
6	Wait	-	-	-	2
7	Elute W1	Solvent 2	5	18	-
8	Wait	-	-	-	1
9	Elute W1	Solvent 2	5	5	-
10	Wait	-	-	-	2
11	Add Sample W1	Sample	10	285	-
12	Rinse W1	Solvent 2	10	7.5	-
13	Rinse W1	Solvent 2	10	7.5	-
14	Add Sample W1	Sample	10	4.5	-
15	Elute W1	Solvent 1	10	0.2	-
16	Air-Purge1	Air	10	5	-
17	Blow N ₂				5 @ 2.0 L/min
18	Rinse 1	Solvent 1	5	4	-
19	Wait	-	-	-	2
20	Rinse 1	Solvent 1	5	4	-
21	Wait	-	-	-	2
22	Collect 1	Sample	5	4.5	-
23	Air-Purge1	Air	5	10	-

LC Conditions

Column: Gemini™ 3 µm C18, 100 x 2.0 mm ([00D-4439-B0](#))
 Luna™ 5 µm C18(2), 30 x 2.0 mm ([00A-4252-B0](#))

Mobile Phase: A: 20 mM Ammonium acetate in water
 B: Methanol

Gradient:	Time (min)	%B
	0	5
	0.1	55
	5.4	99
	9	99
	10	99
	10.1	5
	12	5

Flow Rate: 430 µL/min

Injection Volume: 5 µL

Temperature: 40 °C

LC System: Agilent® 1260 Infinity

Detection: LC-MS/MS

Detector: 6500+ QTRAP® (SCIEX®)

MS Conditions

Ion Source: Negative

Source Temperature: 400 °C

GS1: 40

GS2: 40

CUR: 35

IS: -4500



Table 2. MRM Transitions

Analyte	Q1 (m/z)	Q2 (m/z)
PFBS	298.9	79.9
PFHxA	312.9	268.9
HFPODA	284.8	168.9
PFHpA	362.9	318.9
PFHxS	398.9	79.9
ADONA	376.9	250.9
PFOA	412.9	368.8
PFOS	498.9	79.9
PFNA	462.9	418.9
9CLPF3	530.8	350.9
PFDA	512.9	468.9
MeFOSA	569.9	418.9
PFUnA	562.9	518.9
EtFOSA	583.9	418.9
11CLPF	630.8	450.9
PFDoA	612.8	568.9
PFTTrDA	662.9	618.9
PFTA	712.9	668.9

OCWD's experience with EPA Method 537.1 in a production laboratory setting reveals some interesting contrasts between the economics of manual and automated PFAS sample preparation. The manual preparation allows for 30 sample bottles (total of field and QC samples) to be processed by one technician in a 9 - 10-hour shift. The automated preparation, however, allows for 48 sample bottles (total of field and QC samples) to be processed by one technician in a 9 - 10-hour shift.

These averages suggest that the automated procedure has a 60% higher throughput (per technician, per shift) than that of the manual method, resulting in higher laboratory labor productivity as well as higher sample throughput. In practice, however, the laboratory labor productivity gains can be significantly higher than 60 % because the automated method – once set up and running – allows “walk-away” operation, permitting the technician to go and perform other laboratory duties while the batch of samples is running. In contrast, the manual method, while not always requiring complete analyst attention, does require frequent input and adjustment which restricts the ability of the technician to be absent for longer periods of time. In fact, the greatest quality risk when conducting Method 537.1 manual sample preparation is to allow the SPE column to go dry. Therefore, the technician's time must be closely focused on maintaining SPE batch process integrity.

Of course, the primary barrier to the automation of sample preparation is the high capital cost of the instrumentation which runs in the tens of thousands of dollars, nearly 10X higher than a manual SPE manifold and vacuum pump. At a certain level of sample throughput, the total cost of the automated method (including capital depreciation) becomes lower than that of the manual method on a total \$/sample basis. (Note that the consumable consumption costs of the two approaches are virtually identical on a \$/sample basis.) Therefore, high throughput laboratories tend to migrate to the automated solution and lower throughput laboratories are comfortable staying with the manual method. Each laboratory must make an analysis and buying decision based upon their specific circumstances. However, in either case, the laboratory can be assured that, whether manual or automated, the Strata™ SDB-L SPE cartridges, and Gemini™ C18 and Luna™ C18(2) HPLC columns will provide accurate and precise analytical data.

Results and Discussion

Figure 1 shows a chromatogram for a 2 ng/L calibration standard demonstrating excellent separation of the EPA 537.1 analyte panel. Figure 2 shows a chromatogram of a 2 ng/L Laboratory Fortified Blank (LFB) showing excellent resolution of all analytes near the lower end of the quantitation range. Figures 3-5 present the mean recoveries of 18 PFAS analytes that were spiked into reagent water at levels of 50, 20, and 2 ng/L respectively. The 18 analytes were selected from the suite of 27 analytes to show a broad diversity of compound chemical class and properties. For direct comparison, each analyte is displayed in two color-coded recovery bars. The blue bar designates mean analyte % recovery for the manual extraction process and the red bar designates mean analyte % recovery for the automated SPE-03 extraction process. In Table 3, the recovery data from Figures 3-5 are summarized in tabular form to show the overall comparison of the two techniques at the three spiking levels. The averaged summary of the mean recovery data is presented in Table 4.

The recovery data presented here shows all analytes falling within the acceptable recovery range of >50 % to <150 % for 2 ng/L and >70 % to <130 % for 20 ng/L and 50 ng/L. A casual visual examination of Figures 3-5 also suggests a high degree of consistency between the manual and automated sample preparation approaches with minor, random variations between the two techniques over the full range of concentrations. These observations are confirmed by the tabulated values in Table 3 and by the average recoveries and deviations in Table 4.

As seen in Table 4 there are some minor variations between the two techniques, but these differences are more suggestive than prescriptive. The averages of the standard deviations for both techniques are well below 10 % and are essentially equal. However, the average deviation of the manual technique is slightly more consistent over the full concentration range, whereas the automated technique shows slightly higher (but acceptable) variation at the lower end of the concentration range.

The OCWD has extensive experience in the application of EPA Method 537.1 and estimates that they have analyzed between 5,600 and 6,000 PFAS drinking water samples by EPA Method 537, 537 Version 1.1 and 537.1 since the inception of the 537 method and the UCMR3 program. With the current heightened focus on PFAS in drinking water, they are currently analyzing between 1,800 and 2,000 PFAS sample per year, a rate that is certain to increase with the advent of UCMR5.

Figure 1. HPLC Chromatogram of a 2 ng/L Calibration Standard

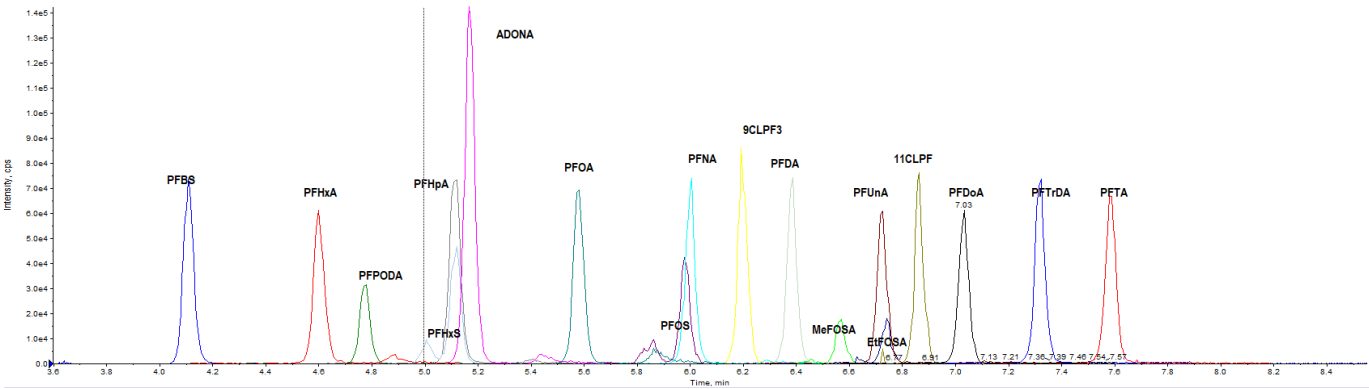


Figure 2. HPLC Chromatogram of a 2 ng/L LFB

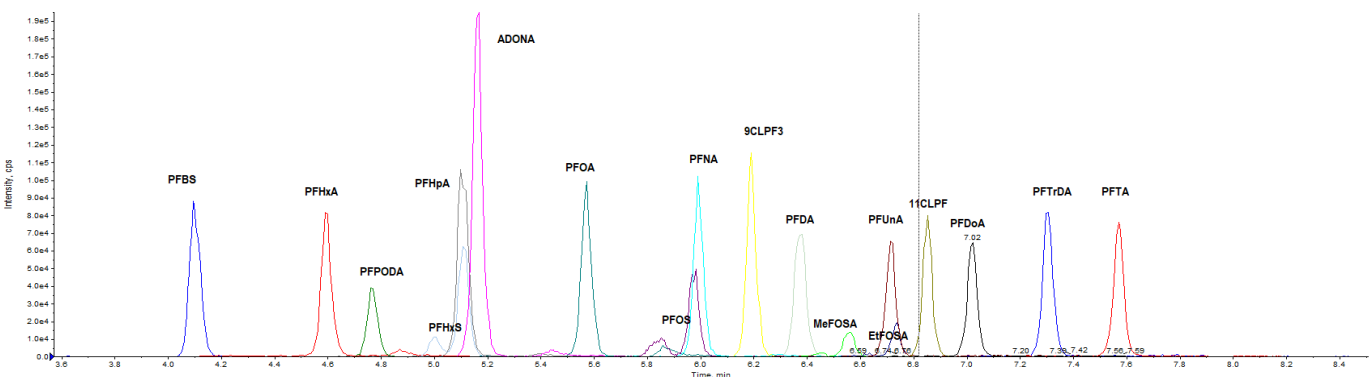


Figure 3. Comparison of Mean Analyte % Recoveries from 50 ng/L LFB, n=19

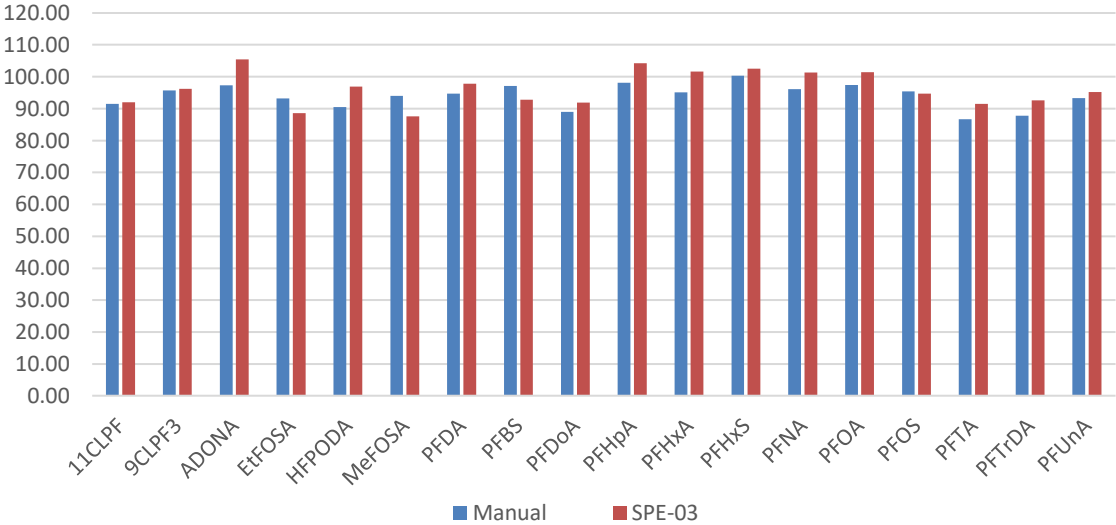


Figure 4. Comparison of Mean Analyte % Recoveries from 20 ng/L LFB, n=19

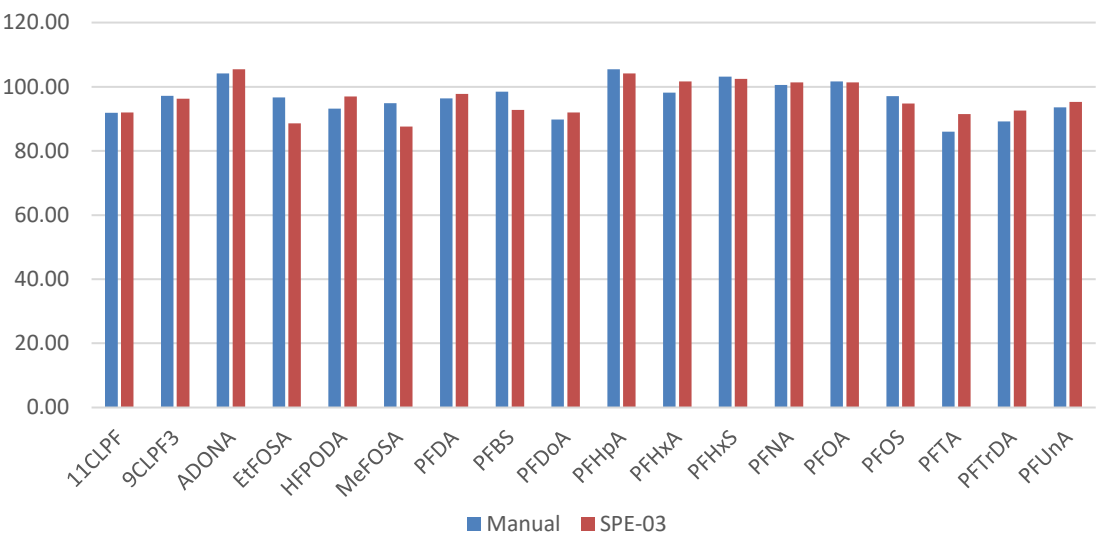


Figure 5. Comparison of Mean Analyte % Recoveries from 2 ng/L LFB, n=19

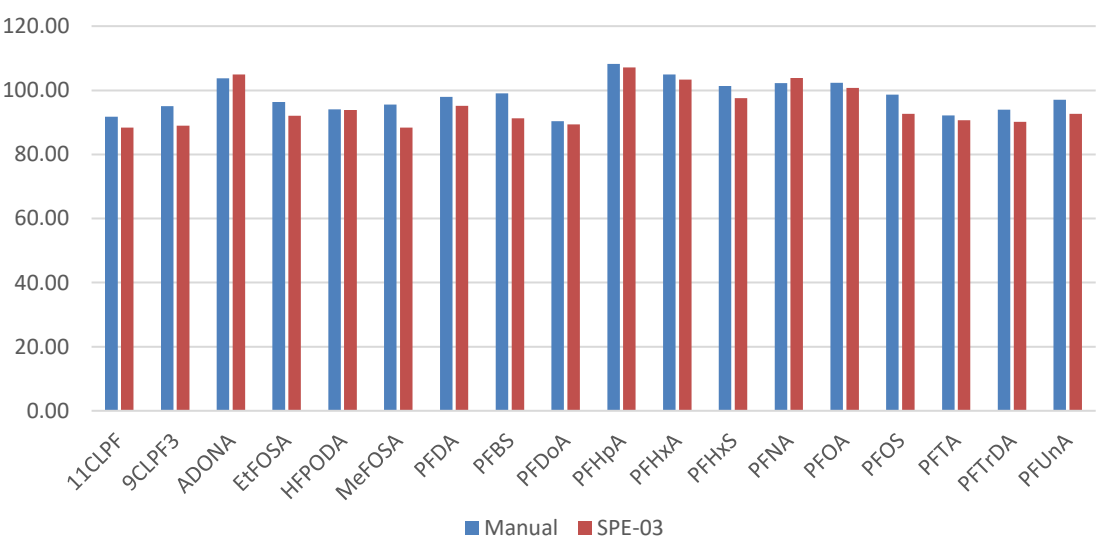


Table 3. Full 18 Analyte Mean Accuracy Comparisons at 50, 20, and 2 ng/L Spiking Levels, n=19

	50 ng/L		20 ng/L		2 ng/L	
Analyte	Manual	Automated	Manual	Automated	Manual	Automated
11CLPF	91.5	92.0	91.3	92.0	91.8	88.3
9CLPF3	95.7	96.2	97.2	96.2	95.1	88.9
ADONA	97.3	105.4	104.1	105.4	103.8	104.9
EtFOSA	93.2	88.6	96.7	88.6	96.4	92.1
HFPODA	90.5	97.0	93.1	97.0	94.1	93.8
MeFOSA	94.0	87.6	94.9	87.6	95.6	88.4
PFDA	94.8	97.8	96.4	97.8	98.0	95.2
PFBS	97.1	92.8	98.5	92.8	99.1	91.2
PFDoA	89.0	91.9	89.8	91.9	90.4	89.4
PFHpA	98.1	104.2	105.5	104.2	108.3	107.1
PFHxA	95.1	101.7	98.2	101.7	104.9	103.3
PFHxS	100.3	102.5	103.1	102.5	101.4	97.6
PFNA	96.1	101.3	100.6	101.3	102.3	103.8
PFOA	97.5	101.4	101.6	101.4	102.4	100.8
PFOS	95.4	94.7	97.0	94.7	98.7	92.7
PFTA	86.7	91.5	86.0	91.5	92.2	90.7
PFTTrDA	87.8	92.6	89.2	92.6	94.0	90.2
PFUnA	93.3	95.2	93.6	95.2	97.0	92.7

Table 4. Average Recovery/Precision Comparison of 50, 20, and 2 ng/L LFB, n=19



	Average % Recovery		Average Standard Deviation	
Spike Concentration	Manual	Automated	Manual	Automated
50 ng/L	94.2	96.4	7.65	6.15
20 ng/L	96.5	96.3	7.58	7.75
2 ng/L	98.1	95.1	7.75	9.29
Overall Average	96.3	95.9	7.66	7.73

Conclusions

Both the manual and the automated sample preparation techniques, when diligently applied, are shown to be acceptable, analytically-equivalent approaches to the performance of EPA method 537.1. The decision of which technique to apply is primarily an economic choice which balances an individual laboratory's need for high sample throughput (with higher capital cost, but lower per sample labor cost) against lower sample throughput (with lower capital cost, but higher per sample labor cost). Whichever approach is chosen, Strata™ SDB-L SPE cartridges, and Luna™ C18(2) and Gemini™ C18 HPLC columns are the logical choice for EPA method 537.1. Phenomenex SPE cartridges and HPLC columns have proven themselves to be the reliable “work horse” of the PFAS testing industry as demonstrated by the successful analysis of hundreds of thousands of environmental PFAS samples.



Strata™ SDB-L (styrene-divinylbenzene) Ordering Information

Format	Sorbent Mass	Part Number	Unit
Tube			
	100 mg	8B-S014-EAK	1 mL (100/box)
	200 mg	8B-S014-FBJ	3 mL (50/box)
	200 mg	8B-S014-FCH	6 mL (30/box)
	500 mg	8B-S014-HBJ	3 mL (50/box)
	500 mg	8B-S014-HCH	6 mL (30/box)
	1 g	8B-S014-JCH	6 mL (30/box)
Giga™ Tube			
	10 g	8B-S014-MFF	60 mL (16/box)
96-Well Plate			
	50 mg	8E-S014-DGB	2 Plates/Box



NEW
PFAS CRM Native Standards
See page 9 for details

Gemini™ pH Flexible LC Columns Ordering Information

3 µm Microbore, Minibore and MidBore™ Columns (mm)										SecurityGuard™ Cartridges (mm)
Phases	50 x 1.0	20 x 2.0	30 x 2.0	50 x 2.0	100 x 2.0	150 x 2.0	50 x 3.0	100 x 3.0	150 x 3.0	4 x 2.0*/10pk
C18	00B-4439-A0	00M-4439-B0	00A-4439-B0	00B-4439-B0	00D-4439-B0	00F-4439-B0	00B-4439-Y0	00D-4439-Y0	00F-4439-Y0	AJ0-7596
C6-Phenyl	—	—	—	00B-4443-B0	00D-4443-B0	00F-4443-B0	00B-4443-Y0	00D-4443-Y0	00F-4443-Y0	AJ0-7914
NX-C18	00B-4453-A0	00M-4453-B0	00A-4453-B0	00B-4453-B0	00D-4453-B0	00F-4453-B0	00B-4453-Y0	00D-4453-Y0	00F-4453-Y0	AJ0-8367

for ID: 2.0-3.0 mm

Luna™ Ordering Information

5 µm Microbore and Minibore Columns (mm)						SecurityGuard™ Cartridges (mm)
Phases	150 x 1.0	30 x 2.0	50 x 2.0	150 x 2.0	250 x 2.0	4 x 2.0* /10pk
Silica(2)	—	00A-4274-B0	00B-4274-B0	00F-4274-B0	00G-4274-B0	AJ0-4347
C5	—	00A-4043-B0	00B-4043-B0	00F-4043-B0	—	AJ0-4292
C8(2)	—	00A-4249-B0	00B-4249-B0	00F-4249-B0	00G-4249-B0	AJ0-4289
C18(2)	00F-4252-A0	00A-4252-B0	00B-4252-B0	00F-4252-B0	00G-4252-B0	AJ0-4286
CN	—	—	00B-4255-B0	00F-4255-B0	—	AJ0-4304
Phenyl-Hexyl	—	00A-4257-B0	00B-4257-B0	00F-4257-B0	00G-4257-B0	AJ0-4350
NH ₂	—	00A-4378-B0	00B-4378-B0	00F-4378-B0	00G-4378-B0	AJ0-4301
SCX	—	—	00B-4398-B0	—	—	AJ0-4307
PFP(2)	—	00A-4448-B0	00B-4448-B0	00F-4448-B0	—	AJ0-8326

for ID: 2.0-3.0 mm

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJ0-4282](#)



PFAS CRM Native Standards. All analytes at the same concentration in acid form for easy calculation and dilution.

Product	Part	Volume	Concentration
EPA 533 mix	ALO-101838	1 mL	2 µg/mL in Methanol
EPA 537.1 mix	ALO-101839	1mL	2 µg/mL in Methanol
EPA 533 + 537.1 mix	ALO-101840	1 mL	2 µg/mL in Methanol

More PFAS Products for Your PFAS Methods

Description	Part No.
Luna™ Omega Column 3 µm PS C18 50 x 3 mm	00B-4758-Y0
Kinetex™ EVO Column 5 µm C18 100 x 2.1 mm	00D-4633-AN
Strata™ PFAS (WAX/GCB) SPE 200 mg, /50 mg, /6mL tubes, 30/pk	CS0-9207
Strata SDB-L 500 mg/6mL tubes, 30/pk	8B-S014-HCH
Verex™ Vial, 9 mm Screw, PP, 1.7 mL, 1000/pk	AR0-39P0-13
Verex Vial, 9 mm Screw, PP, 300 µL, 1000/pk	AR0-39P2-13
Verex Vial, 9 mm Screw, PP, 700 µL, 1000/pk	AR0-39P1-13
Vial Cap Verex™ Cert+ Cap (one piece), 9 mm, PE w/ Starburst pre-Slit, 2mL, 1000/pk	AR0-89P6-13-C



Need a different column size or sample preparation format?

No problem! We have a majority of our available dimensions up on www.phenomenex.com, but if you can't find what you need right away, our super helpful Technical Specialists can guide you to the solution via our online chat portal www.phenomenex.com/Chat.

Australia

t: +61 (0)2-9428-6444
auinfo@phenomenex.com

Austria

t: +43 (0)1-319-1301
anfrage@phenomenex.com

Belgium

t: +32 (0)2 503 4015 (French)
t: +32 (0)2 511 8666 (Dutch)
beinfo@phenomenex.com

Canada

t: +1 (800) 543-3681
info@phenomenex.com

China

t: +86 400-606-8099
cninfo@phenomenex.com

Czech Republic

t: +420 272 017 077
cz-info@phenomenex.com

Denmark

t: +45 4824 8048
nordicinfo@phenomenex.com

Finland

t: +358 (0)9 4789 0063
nordicinfo@phenomenex.com

France

t: +33 (0)1 30 09 21 10
franceinfo@phenomenex.com

Germany

t: +49 (0)6021-58830-0
anfrage@phenomenex.com

Hong Kong

t: +852 6012 8162
hkinfo@phenomenex.com

India

t: +91 (0)40-3012 2400
indiainfo@phenomenex.com

Indonesia

t: +62 21 5019 9707
indoinfo@phenomenex.com

Ireland

t: +353 (0)1 247 5405
eireinfo@phenomenex.com

Italy

t: +39 051 6327511
italiainfo@phenomenex.com

Japan

t: +81 (0) 120-149-262
jpinfo@phenomenex.com

Luxembourg

t: +31 (0)30-2418700
nlinfo@phenomenex.com

Mexico

t: 01-800-844-5226
tecnicomx@phenomenex.com

The Netherlands

t: +31 (0)30-2418700
nlinfo@phenomenex.com

New Zealand

t: +64 (0)9-4780951
nzinfo@phenomenex.com

Norway

t: +47 810 02 005
nordicinfo@phenomenex.com

Poland

t: +48 22 104 21 72
pl-info@phenomenex.com

Portugal

t: +351 221 450 488
ptinfo@phenomenex.com

Singapore

t: +65 6559 4364
sginfo@phenomenex.com

Slovakia

t: +420 272 017 077
sk-info@phenomenex.com

Spain

t: +34 91-413-8613
espinfo@phenomenex.com

Sweden

t: +46 (0)8 611 6950
nordicinfo@phenomenex.com

Switzerland

t: +41 (0)61 692 20 20
swissinfo@phenomenex.com

Taiwan

t: +886 (0) 0801-49-1246
twinfo@phenomenex.com

Thailand

t: +66 (0) 2 566 0287
thaiinfo@phenomenex.com

United Kingdom

t: +44 (0)1625-501367
ukinfo@phenomenex.com

USA

t: +1 (310) 212-0555
www.phenomenex.com/chat

🌐 **All other countries/regions**
Corporate Office USA

t: +1 (310) 212-0555
www.phenomenex.com/chat

www.phenomenex.com

Phenomenex products are available worldwide. For the distributor in your country/region, contact Phenomenex USA, International Department at international@phenomenex.com

BE-HAPPY™
GUARANTEE

Your happiness is our mission. Take 45 days to try our products. If you are not happy, we'll make it right.

www.phenomenex.com/behappy

Terms and Conditions

Subject to Phenomenex Standard Terms and Conditions, which may be viewed at www.phenomenex.com/TermsAndConditions.

Trademarks

Strata, Gemini, Verex, Kinetex, Luna, MidBore, Giga, SecurityGuard, and BE-HAPPY are trademarks of Phenomenex. Agilent is a registered trademark and Vac Elut is a trademark of Agilent Technologies, Inc.

QTRAP and SCIEX are registered trademarks of AB SCIEX Pte. Ltd. Milli-Q is a registered trademark of Merck KGaA, Darmstadt, Germany.

Disclaimer

Comparative separations may not be representative of all applications.

SecurityGuard is patented by Phenomenex. U.S. Patent No. 6,162,362

CAUTION: this patent only applies to the analytical-sized guard cartridge holder, and does not apply to SemiPrep, PREP, or ULTRA holders, or to any cartridges.

Phenomenex is in no way affiliated with Orange County Water District, PromoChrom Technologies or Agilent Technologies, Inc.

FOR RESEARCH USE ONLY. Not for use in clinical diagnostic procedures.

© 2022 Phenomenex, Inc. All rights reserved.

