

## Yarra 3µm SEC-3000 3 batch overlay PMQC Conditions

**Column:** Yarra™ 3 µm SEC-3000, LC Column 300 x 7.8 mm, Ea

**Dimensions:** 300 x 7.8 mm ID

**Order No:** 00H-4513-K0

**Elution Type:** Isocratic

**Eluent A:** 100 mm PO4 Buffer pH 6.8 100 mm Sodium Phosphate in Water pH 6.8 with 0.025% NaI


Gradient Profile:	Step No.	Time (min)	Pct A
	1	0	100

**Flow Rate:** 1 mL/min

**Col. Temp.:** ambient

**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 280 nm (ambient)

20632

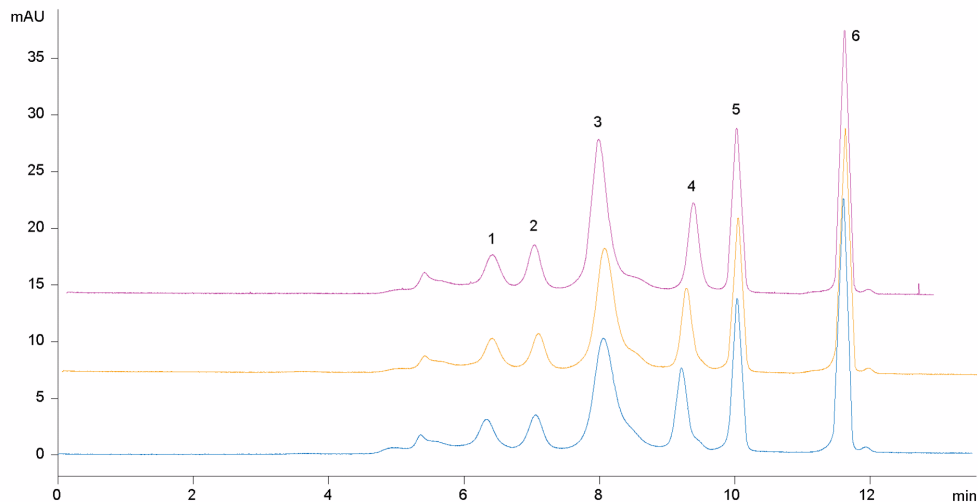

### ANALYTES:

- 1** Thyroglobulin (669kDa)  
Retention Time: 6.4 min
- 2** IgA (300kDa)  
Retention Time: 7 min
- 3** IgG (150kDa)  
Retention Time: 8 min
- 4** Ovalbumin (44kDa)  
Retention Time: 9.2 min
- 5** Myoglobin  
Retention Time: 10 min
- 6** Uridine  
Retention Time: 11.5 min



Products used in this application:

